

Understanding metrological traceability in calibration

Metrological traceability is an important part of measurement. One of the best ways to understand an instrument's measurement performance is to assess its accuracy. The instrument should be calibrated against an SI-traceable reference to ensure the quality of measurement data. Quality data, in turn, provides reliable information for decision making.

National Metrology Institutes (NMI) create SI units with detailed and analyzed uncertainties. The units are then transferred to secondary standards (e.g. to accredited laboratories) for use in calibrations. The traceability chain for industrial instruments is established through calibration against the secondary standards. Finally, the manufactured measurement instrument is calibrated against the industrial standard with a calculated uncertainty. Thus, an unbroken and documented chain of calibrations to the SI unit is achieved. Measurement values from the manufactured instrument is considered to be SI-traceable with a known uncertainty.

The more calibration steps there are between the SI unit and the manufactured instrument, the greater the measurement uncertainty. Ideally, the chain of traceability in calibrations should be as short as possible for demanding applications.

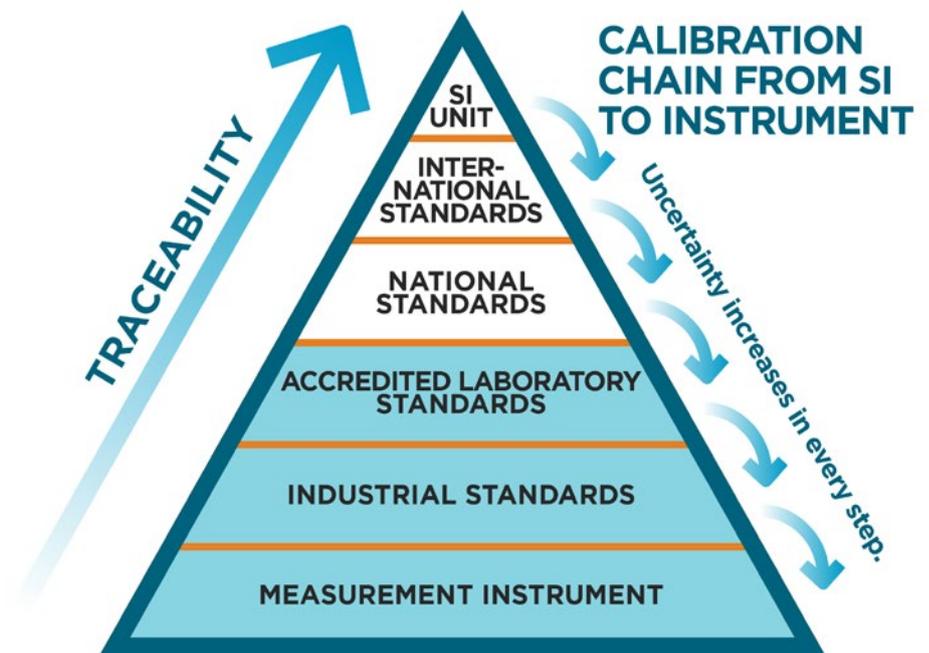


Figure 1: Metrological traceability (Calibration Chain) from an SI unit to a measurement instrument. Blue shading indicates the level of traceability of Vaisala instruments.

Assessing traceability

How do you know if your instrument is indeed SI-traceable? One way is to study its calibration certificate. For example, the following information should be available:

- 1 Calibration results include measurement uncertainties
- 2 All calibration references are identified
- 3 Notes on how uncertainties are determined and what uncertainty sources are included
- 4 Description of how the SI traceability was established
- 5 Reference and ambient conditions

Sample calibration certificate

3

The H₂O₂ measurement of HPP272 was calibrated by comparing the instrument's H₂O₂ readings to a generated reference H₂O₂ reading. The reference H₂O₂ reading was calculated based on reference equipment measurement results: H₂O₂ liquid flow, H₂O₂ liquid density, nitrogen flow, gas pressure and temperature.

4

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2$, which for a normal distribution corresponds to a coverage probability of approximately 95 %. The measurement results are traceable to the international system of units (SI) through national metrology institutes (NIST USA, MIKES Finland, or equivalent) or via ISO/IEC 17025 accredited calibration laboratories.

1

Hydrogen peroxide results

Reference H ₂ O ₂ [ppm]	Observed H ₂ O ₂ [ppm]	H ₂ O ₂ Error [ppm]	Acceptance Limit [ppm]	Pass/Fail
499	489	-10	±25	Pass
997	997	0	±50	Pass

Relative saturation results

Reference Relative Saturation [%RS]	Observed Relative Saturation [%RS]	Relative Saturation Error [%RS]	Acceptance Limit [%RS]	Pass/Fail
11.1	11.3	0.2	±3.0	Pass
35.3	36.3	1.0	±4.0	Pass

Reference equipment used in calibration

Type	Identity Number	Certificate Number	Calibration Date	Calibration Due Date
Liquid pump	18156	C03898	2019-11-21	2020-05-31
Pressure and temperature	19273	K008-C01855	2019-06-04	2020-06-30
Pressure and temperature	19274	K008-C01854	2019-06-04	2020-06-30
Density meter	17897	H92-194620001	2019-11-12	2020-11-30
Mass flow controller	MF 13700	C04239	2019-12-19	2020-12-31
Mass flow controller	17894	D01569	2020-05-05	2021-05-31
Mass flow meter	17896	C03716	2019-11-01	2020-11-30

2

Calibration uncertainty ($k=2$, ~95% confidence level):

H₂O₂

Concentration ± 10 ppm @ 500 ppm, ± 20 ppm @ 1000 ppm

RS

Relative saturation ± 2 %RS @ 10 %RS, ± 4 %RS @ 40 %RS

1

5

Ambient conditions:

Humidity [%RH] Temperature [°C] Pressure [hPa]
 28 ± 4 22 ± 2 1007 ± 20

Figure 2: Factory calibration certificate for Vaisala's HPP272 hydrogen peroxide probe.

Calibration should match the application

A manufactured instrument can have SI-traceable calibration even though it was not calibrated in an accredited laboratory. Typically, calibration certificates provided by instrument manufacturers include these kinds of calibrations.

In the worst-case scenario, calibrations may not actually be SI-traceable. Documentation indicating the SI traceability chain should always be available to the instrument end user. At Vaisala this is a standard for every product.

It is helpful, especially for demanding applications, to understand what you are looking for in terms of calibration references and measurement uncertainties.

VAISALA

Please contact us at
www.vaisala.com/contactus



Scan the code for more information

Ref. B212197EN-A ©Vaisala 2020

This material is subject to copyright protection, with all copyrights retained by Vaisala and its individual partners. All rights reserved. Any logos and/or product names are trademarks of Vaisala or its individual partners. The reproduction, transfer, distribution or storage of information contained in this brochure in any form without the prior written consent of Vaisala is strictly prohibited. All specifications – technical included – are subject to change without notice.

www.vaisala.com